



PCT/GB 2003 / 0 0 3 5 2 4
Rec'd PCTO 15 JUL 2005
10/542257
INVESTOR IN PEOPLE

PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN
COMPLIANCE WITH RULE 17.1(a) OR (b)

The Patent Office
Concept House
Cardiff Road
Newport
South Wales
NP10 8QQ

REC'D 25 SEP 2003


WIPO PCT

I, the undersigned, being an officer duly authorised in accordance with Section 74(1) and (4) of the Deregulation & Contracting Out Act 1994, to sign and issue certificates on behalf of the Comptroller-General, hereby certify that annexed hereto is a true copy of the documents as originally filed in connection with the patent application identified therein.

In accordance with the Patents (Companies Re-registration) Rules 1982, if a company named in this certificate and any accompanying documents has re-registered under the Companies Act 1980 with the same name as that with which it was registered immediately before re-registration save for the substitution as, or inclusion as, the last part of the name of the words "public limited company" or their equivalents in Welsh, references to the name of the company in this certificate and any accompanying documents shall be treated as references to the name with which it is so re-registered.

In accordance with the rules, the words "public limited company" may be replaced by p.l.c., plc, P.L.C. or PLC.

Re-registration under the Companies Act does not constitute a new legal entity but merely subjects the company to certain additional company law rules.

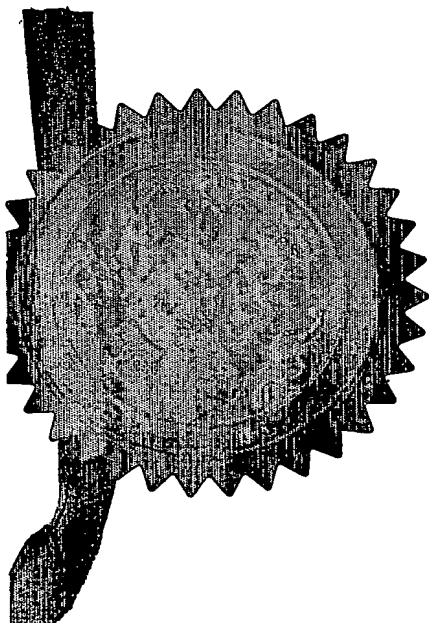

Signed

Dated

17 September 2003



1/77

Request for grant of a patent

(See the notes on the back of this form. You can also get an explanatory leaflet from the Patent Office to help you fill in this form)

The Patent Office

Cardiff Road,
Newport
South Wales
NP10 8QQ

1. Your reference P17001GB-H/JCC/lp

2. Patent application number 0301047.7
(The Patent Office will fill in this part)

17JAN03 E777769-3 000389
P01/7700 0.00-0301047.7

3. Full name, address and postcode of the or of each applicant (underline all surnames)
Thermo Shandon Limited,
93-96 Chadwick Road,
Astmoor,
RUNCORN,
Cheshire WA7 1PR

16 JAN 2003

Patents ADP number (if you know it)

8194227001

If the applicant is a corporate body, give the country/state of its incorporation

4. Title of the invention
A Centrifugation Device

5. Name of your agent (if you have one)
Forrester Ketley & Co.
"Address for service" in the United Kingdom to which all correspondence should be sent (including the postcode)
Forrester House
52 Bounds Green Road
London
N11 2EY

Patents ADP number (if you know it)

133001

6. If you are declaring priority from one or more earlier patent applications, give the country and the date of filing of the or of each of these earlier applications and (if you know it) the or each application number	Country	Priority application number (if you know it)	Date of filing (day / month / year)
--	---------	---	--

7. If this application is divided or otherwise derived from an earlier UK application, give the number and the filing date of the earlier application	Number of earlier application	Date of filing (day / month / year)
---	-------------------------------	--

8. Is a statement of inventorship and of right to grant of a patent required in support of this request? (Answer 'Yes' if:

a) any applicant named in part 3 is not an inventor, or

b) there is an inventor who is not named as an applicant, or

c) any named applicant is a corporate body.

See note (d))

YES

Patents Form 1/77

9. Enter the number of sheets for any of the following items you are filing with this form. Do not count copies of the same document

Continuation sheets of this form

Description

8

Claim(s)

-

Abstract

-

Drawing(s)

6

10. If you are also filing any of the following, state how many against each item.

Priority documents

Translations of priority documents

Statement of inventorship and right to grant of a patent (*Patents Form 7/77*)

Request for preliminary examination and search (*Patents Form 9/77*)

Request for substantive examination (*Patents Form 10/77*)

Any other documents
(please specify)

11.

I/We request the grant of a patent on the basis of this application.

Signature

Forrester Ketley & Co

Date

16 January 2003

Forrester Ketley & Co.

12. Name and daytime telephone number of person to contact in the United Kingdom

(020) 8889 6622

C.A. HOWDEN

Warning

After an application for a patent has been filed, the Comptroller of the Patent Office will consider whether publication or communication of the invention should be prohibited or restricted under Section 22 of the Patents Act 1977. You will be informed if it is necessary to prohibit or restrict your invention in this way. Furthermore, if you live in the United Kingdom, Section 23 of the Patents Act 1977 stops you from applying for a patent abroad without first getting written permission from the Patent Office unless an application has been filed at least 6 weeks beforehand in the United Kingdom for a patent for the same invention and either no direction prohibiting publication or communication has been given, or any such direction has been revoked.

Notes

- If you need help to fill in this form or you have any questions, please contact the Patent Office on 08459 500505.
- Write your answers in capital letters using black ink or you may type them.
- If there is not enough space for all the relevant details on any part of this form, please continue on a separate sheet of paper and write "see continuation sheet" in the relevant part(s). Any continuation sheet should be attached to this form.
- If you have answered 'Yes' Patents Form 7/77 will need to be filed.
- Once you have filled in the form you must remember to sign and date it.
- For details of the fee and ways to pay please contact the Patent Office.

THIS INVENTION relates to a centrifugation device comprising a combined sample chamber and slide holder adapted to be mounted, with a microscope slide, in a centrifuge in a predetermined position, after placing, in the sample chamber, a fluid biological sample containing cells, the device being
5 so-arranged that when the centrifuge is operated, a thin layer - ideally a monolayer - of cells is deposited from the fluid onto a predetermined deposition area on the glass microscope slide. Such a centrifugation device is herein referred to as being "of the kind specified".

10 Various forms of centrifugation device of the kind specified have been known in the past. Examples of such devices are disclosed, for example, in US Patents 4,391,710; 4,696,743; 4,853,188 and 4,874,582 and European Patents Nos. 0184374 and 0047840. Some examples have been reusable, that is to say it was possible and intended that after the device had been used to deposit cells
15 from a fluid sample onto a first microscope slide, and the slide removed, the device could be cleaned, a fresh slide fitted, a fresh fluid sample placed in the sample chamber and the device again placed into the centrifuge and so on indefinitely. In these arrangements the slide is, of course retained by a releasable and re-attachable clip of some description. Some later centrifugation
20 devices of the kind specified were of the single-use type, that is to say they were designed in such a way that they could not, or could not conveniently, be used more than once, thereby avoiding contamination problems resulting from improper cleaning procedures between uses. In view of their inevitably disposable nature, devices of the latter character have generally been largely of
25 plastics in order to minimise production costs.

It is an object of the present invention to provide an improved centrifugation device of the single use type.

According to one aspect of the present invention there is provided a centrifugation device as herein defined comprising an integrally moulded body affording a base adapted for engagement with a microscope slide, structure on one side of the base defining a chamber for a fluid sample, with an opening for the introduction of fluid to said chamber, the base including an aperture and carrying a means for sealing the edges of such aperture with respect to the surface of a microscope slide placed across the base, or for allowing the passage of liquid but obstructing the passage of cells, the centrifugation device further including a back plate connected with the base plate by an integral hinge and a latch mechanism formed integrally with the remainder of the device and arranged, when the back plate is closed against the rear of a microscope slide engaged with the base, to locate the slide between the base and the cover plate and to hold the cover plate in this closed position until fracture of a retaining element from the integrally moulded body.

The catch arrangement preferably comprises a detent carried by the back plate adjacent the free edge of the latter and which, in operation, co-operates, in the closed position of the device, with a complementary latch carried by the body of the device and connected with said body by an integral live hinge, the catch arrangement further comprising a shield element which, in the condition of the device before use, is secured in a position in which it extends over the complementary latch at a predetermined distance from the integral live hinge of the said complementary latch, the arrangement being such that in the closed position, with the shield element still attached, the detent on the back plate is retained between the shield element and the complementary latch and the shield element counteracts a turning moment applied to the complementary latch as a result of tension in the back plate detent, whilst on breaking of a frangible retaining element holding the shield member in position relative to the device

body, the shield element is able to move away from said complementary latch allowing the latter to swing away from the back plate detent for release of the back plate detent to allow the back plate to swing away from the body of the device, and to allow removal of the microscope slide.

5

The complementary latch may be provided with a retaining arm which engages a face of the detent on the back plate to push the detent across the abutment face of the latch as the latch tilts outwardly and backwards during the release of the detent after rupture of the connection of the shield member with the body part, and thus to ensure release of the detent from the latch.

10

An embodiment of the invention is described below by way of example with reference to the accompanying drawings in which:

15

Figure 1 is a perspective view, from the rear and above, of a centrifugation device in accordance with the invention in the condition in which a back plate is closed against a body part with a microscope slide located therebetween;

20

Figure 2 is a view in vertical section through the device and microscope slide of Figure 1;

Figure 3 is a perspective view corresponding to Figure 1 but showing the device with the back plate in an open position in relation to the body part, without the microscope slide;

25

Figure 4 is a perspective view corresponding to Figure 3 but from the front and below;

Figure 5 is a perspective view from the rear and below of the device with the back plate in an open position with respect to the body part of the device;

Figure 6 is a partial view in horizontal section, and to an enlarged scale, through the device of Figures 1 to 4, along the line VI - VI in Figure 1 showing details of the catch arrangement, in the closed condition of the back plate,

Figure 7 is a corresponding partial section of view in the open condition of the back plate and

Figure 8 is a fragmentary rear elevation view, also to an enlarged scale, of the body part of the device showing the parts of the catch arrangement carried thereby.

Referring to Figures 1 to 4, a centrifugation device in accordance with the present invention comprises a body part 10 and a back plate 12 formed integrally with one another by moulding in a suitable plastics material such as polypropylene, the back plate 12 being connected with the body part 10 by way of an integral "living hinge" 22. As shown in Figures 3 to 5, the body part 10 comprises a generally planar base or flange 14 which carries on its front side integral structure providing a sample chamber 16 which is closed at its end remote from the base 14 and which terminates, in the plane of the base 14, in a port 18 which, in the preferred embodiment, is rectangular. A funnel 15 extends upwardly from an entrance opening in the sample chamber, whereby a fluid sample can be introduced into the sample chamber 16. As shown in Figures 2 and 3, a resilient gasket, for example of an injection mouldable elastomer, referenced 20 in Figures 2 and 3 is carried by the base 14. The gasket 20 extends around the port 18 and protrudes slightly rearwardly from the rear face of the base 14, for sealing against the adjacent surface of glass microscope slide (26, Figure 2). The material of the gasket 20 is preferably a thermoplastic elastomer such as Evoprene G936, and is moulded in situ on the backplate, the body 10 and integral backplate 12 and the gasket being formed by a two shot injection moulding technique, with the body 10 and backplate being formed in one shot and the gasket being formed in the other shot. The

gasket incorporates an oil component which, in use, forms a thin oil film on the slide 26 where the gasket contacts the slide. This film acts as a barrier to the aqueous fluid of the biological sample and tends to prevent migration of such fluid, from the cell layer deposited on the slide, beyond the boundary defined by the region of contact of the gasket, after opening of the centrifugation device and removal of the side. Subsequent processing of the slide and sample layer generally involves immersion of the slide in an alcohol based medium which also removes the thin oil film.

10 The base 14 is generally rectangular, as is the back plate 12, and the living hinge 22 extends along one vertical edge of the base 14 and the adjacent vertical edge of the back plate 12. The vertical edge of the back plate 12 remote from the living hinge 22 carries a detent 24 for co-operating with elements carried by the body 10 adjacent the edge of the base 14 remote from the living hinge 22 and which elements, together with detent 24, form a catch arrangement whereby the back plate may be secured in a closed position on the base 14 with a microscope slide, indicated at 26 in Figures 1 and 2, held between the base 14 and the back plate 12. As illustrated in Figures 1 to 5, the upper edge of the back plate 12 may be scalloped or recessed, as indicated, to allow ready grasping of the upper edge of the microscope slide 26 between finger and thumb during removal of the slide from the device after centrifugation, as described below.

25 In use of the device, a microscope slide is located between the back plate 12 and the base 14: (Figures 3 and 5 show integral hooks 31 to support the lower end of a microscope slide 26 fitted against the front surface of the back plate 12 until the back plate 12, with the slide, is closed against the base 14). In this condition, as illustrated in Figure 2, the gasket 20 engages the adjacent surface of the slide 26 in a sealing-tight manner.



The device is then mounted in a centrifuge (not shown) in such a manner that bosses 30 projecting from the sides of the back plate act as journals received in bearings provided by complementary slots in mounting structure within the centrifuge. When the centrifuge is at rest, the device rests in the centrifuge in a position in which the slide 26 is at an angle. When the centrifuge is spun up, the device pivots about the axis of bosses 30, into a position in which the slide is vertical. When the centrifuge is spun, the centrifugal force generated produces a rapid settling of the cells within the biological sample against the surface of the glass slide 26, within an area bounded by gasket 20 and these cells remain in a thin layer on the slide after the centrifuge is stopped. In order to ensure a more even distribution of cells across the exposed area of the slide during the centrifuging step, the sample chamber has a plurality of parallel baffle plates 17 extending alternately from opposite sides of the sample chamber, part-way across the latter and generally parallel with the bottom wall of the sample chamber. After the centrifuge is stopped, the centrifugation device removed from the centrifuge, and the slide carefully removed after opening of the back plate as described below.

Referring to Figures 6, 7 and 8, the fragmentary horizontal section views of Figure 6 and Figure 7 show a portion of the back plate 12 adjacent the edge carrying the detent 24 and show the adjacent portion of the body 10 and a latch 32 which is connected with the remainder of the body 10 by an integral live hinge 34. The detent 24 comprises a head portion connected with the adjacent edge of the backplate 12 by a relatively flexible arm 33. The body 10 also carries an integrally formed shield element 36 in the form of a generally flat plate which is disposed at a predetermined distance from the adjoining side wall of the body 10 and extends over the latch 32. There is thus defined between the latch 32 and the shield element 36 a narrow space through which the detent 24 is projected in the closed condition of the back plate shown as Figure 6. In this

position, an abutment surface of the detent 24, facing away from the free end or nose of the detent 24 engages an opposing abutment face of the latch element 32 and, additionally, the surface of the nose of the detent facing away from the shield element 36 is engaged by an opposing surface of the latch 32, afforded
5 by an extension 32A. When the back plate is moved from the open position shown in Figure 7 to the closed position shown in Figure 6, the natural resilience of the living hinge 34 causes the latch 32, originally deflected downwards by the nose of the detent 24, to spring back again into the locking position shown in Figure 6. In this closed position, deflection of the detent 24
10 away from the part of the body 10 to which the hinge 34 is attached, being deflection such as would allow disengagement of the detent 24 from the latch 32, is prevented by engagement of the detent 24 with the shield element 36.

As a result of the arrangement described, it is not possible to open the
15 back plate 12 without removal or displacement of the shield element 36 which, as described below, necessarily involves rupture of a connecting element. As indicated in Figure 8, the shield element 36 conveniently takes the form of a lever having a free end 36A and pivotally connected with a projection 37 from the body 10 by way of an integral living hinge 40. The end of the lever 36
20 remote from free end 36A is secured by a narrow and hence weakened connection 42 to the side of body 10. When it is desired to release the back plate 12 for removal of the slide 26, the free end 36A of the shield element 36 is pressed manually towards the adjacent surface of the body part 10 causing the opposite end of the lever 36 to break from its connection 42 with the body
25 part 10, allowing the portion of the element 36 overlying the detent 24 to move away from the latter allowing the latch 32 to swing backwards and away from the adjoining side wall of the body 10, with corresponding flexure of the arm 33 of the detent away from said side part. The leg 32A, engaging the opposing surface of the detent 24, has the function of forcing detent 24 upwards (as

viewed in Figure 6) as the latch 32 swings backwards, thereby to assist in disengaging the abutment face of the detent 24 from the opposing abutment face of the latch 32. Of course, after fracture of the connection 42 in the manner described, the latch arrangement described cannot be used to hold the
5 back plate 12 in a fully closed position relative to the body part, thus ensuring that the centrifugation device is a single use device.

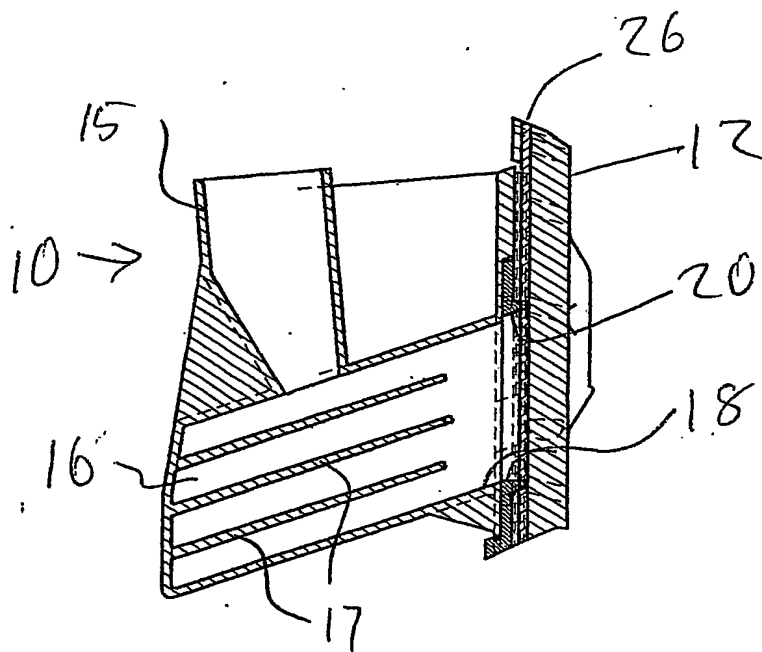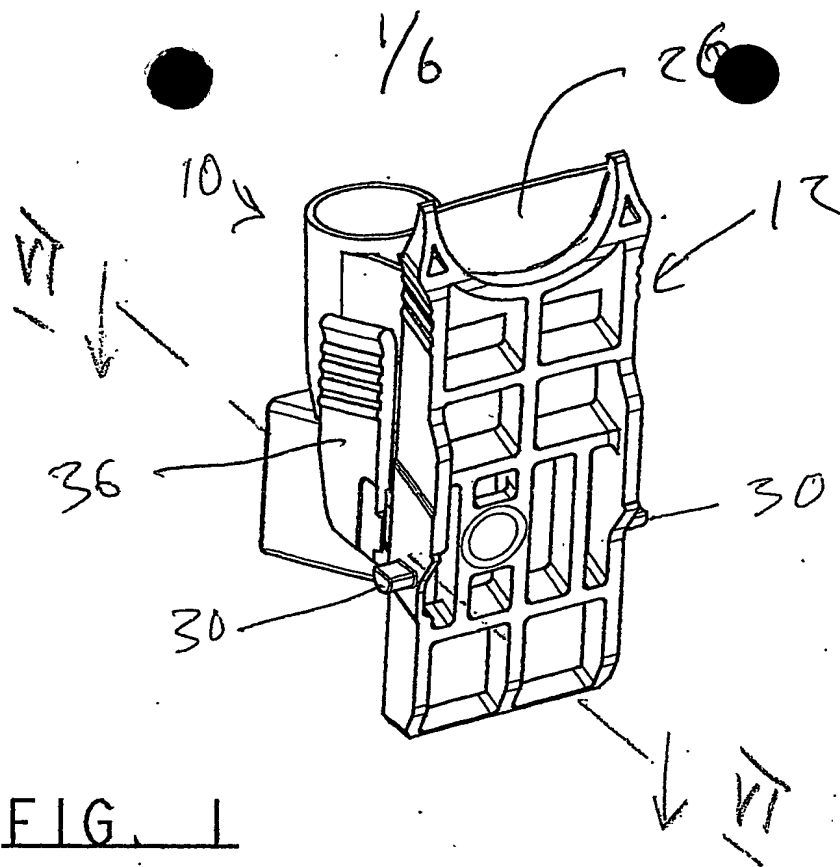

2/6

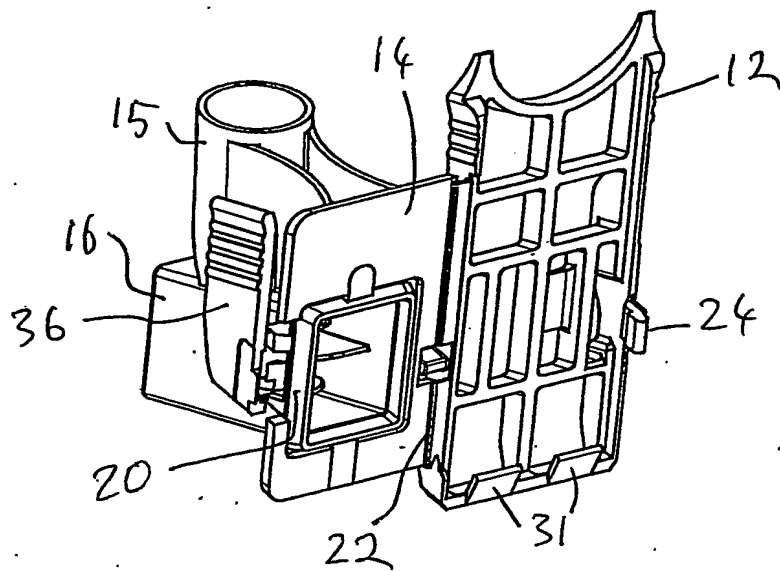


Fig 3

3/6

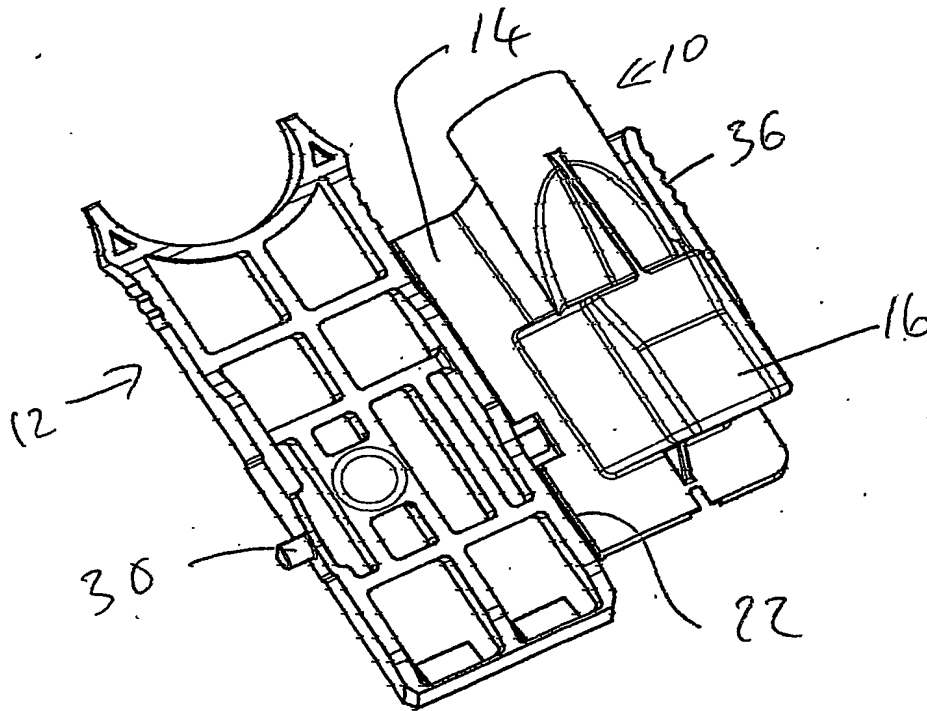


FIG. 4

4/6

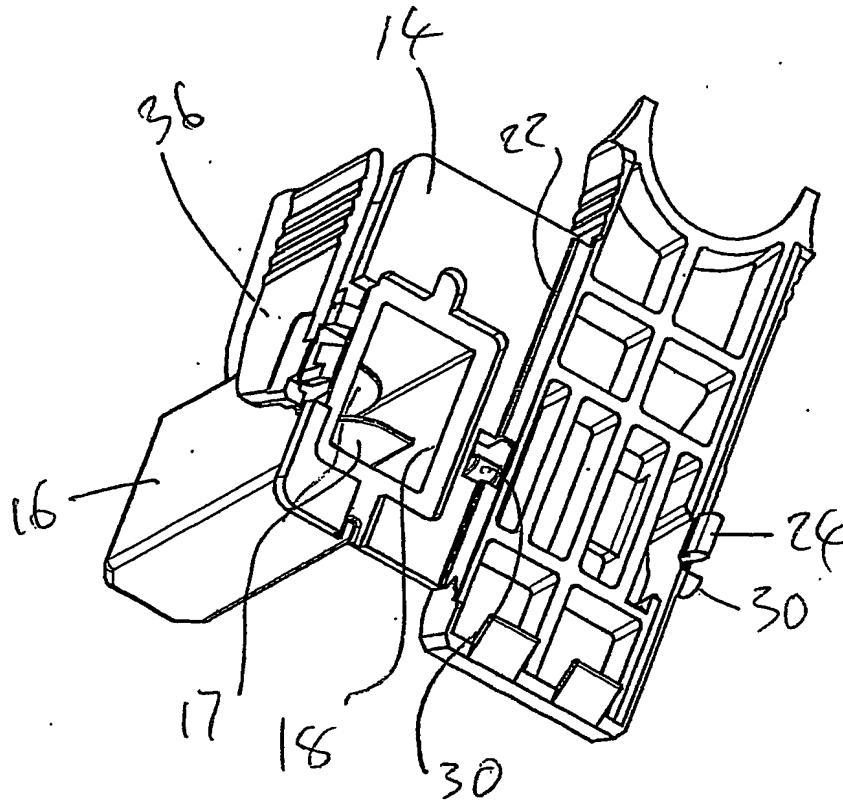


FIG. 5

Fig 6


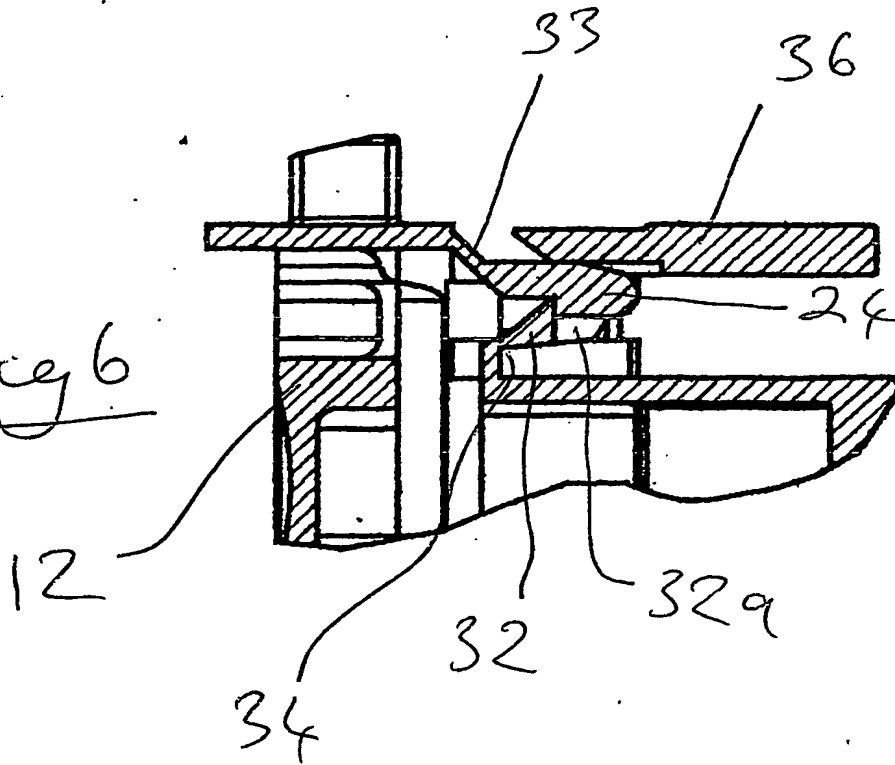


Fig 7

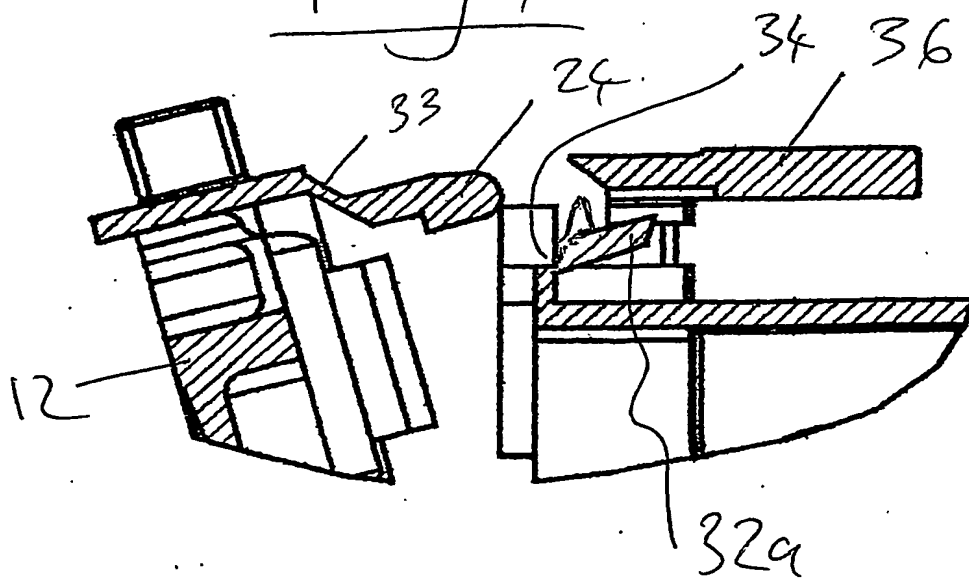

6/6

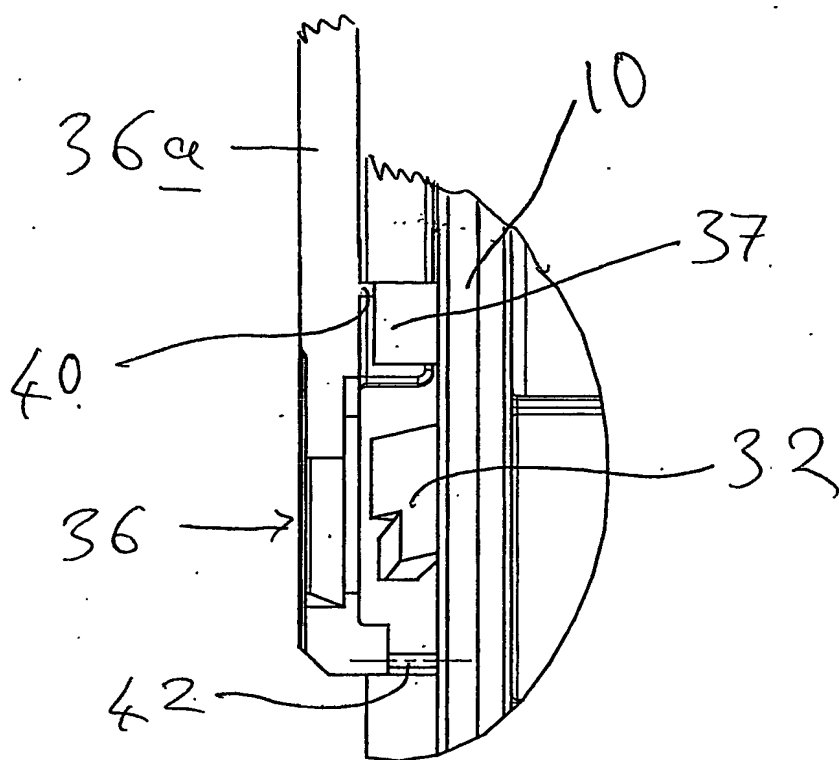


Fig 8